


-15kV TOF: -9116 v  
 -3.6kV MCP: -2169 v  
 -2.4kV MCP: -1579 v  
 Input Cur: 300 ma  
 RPA max: 237 v  
 Mirror max: 238 v

Mon Sep 25 10:47:00 2006

## TIDE Direct Events

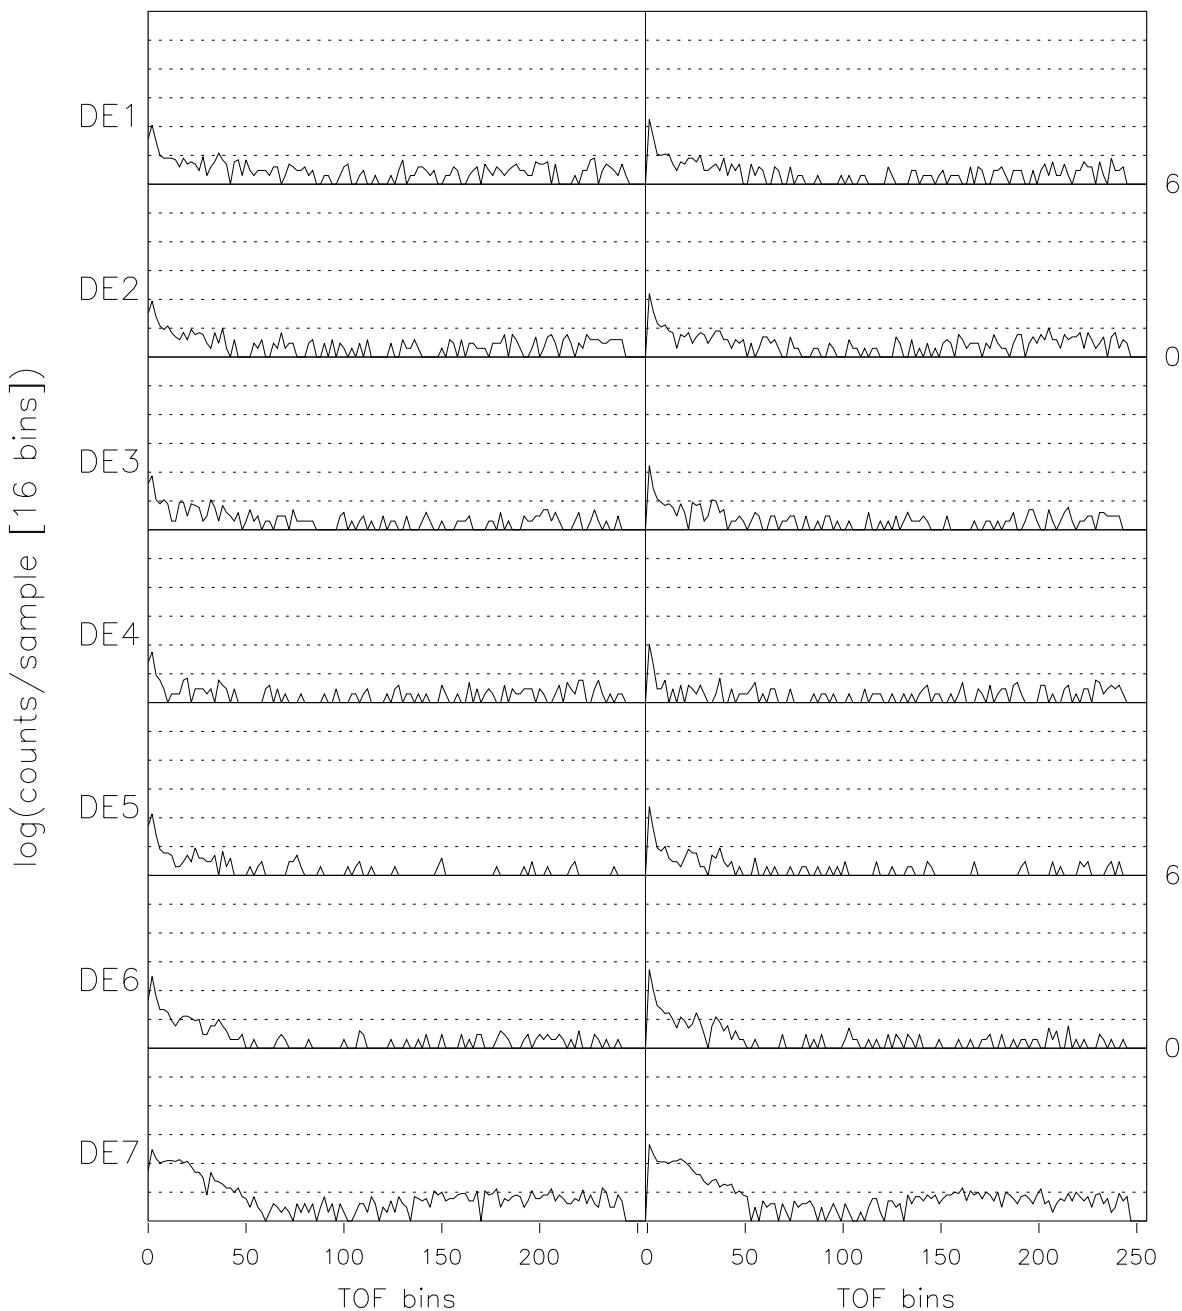

reported: 09-03-96 15:25:24 UT

reported: 09-03-96 15:28:36 UT

file: /export/data/tide/nrt/96090301.dat

-15kV TOF: -9116 v

-3.6kV MCP: -2593 v

-2.4kV MCP: -1589 v

Input Cur: 302 ma

RPA max: 237 v

Mirror max: 238 v